# **DeviceNET®**

Ranges: 0-75 to 0-550 inches

**Industrial Grade** 

# **Specification Summary:**

#### **GENERAL**

Full Stroke Range Options—on this datasheet	0-75 to 0-550 inches
Electrical Signal Interface	CANbus ISO 11898
Protocol	DeviceNET Version 2.0
Accuracy	± 0.10% full stroke
	± 0.02% full stroke
Resolution	± 0.003% full stroke
Measuring Cable Options	nylon-coated stainless steel or thermoplastic
Enclosure Material	powder-painted aluminum or stainless steel
Sensor	plastic-hybrid precision potentiometer
Potentiometer Cycle Life25	50,000, min. –before signal degradation can occur
Maximum Retraction Acceleration	see ordering information
Maximum Velocity	see ordering information
Weight, Aluminum (Stainless Steel) Enclose	ıre 8 lbs. (16 lbs.) max.

#### **ELECTRICAL**


Input Voltage	bus powered
Input Current	
Address Setting/Node ID	063 set via DIP switches -default setting: 63
Baud Rate	125K, 250K or 500K set via DIP switches
EDS File	. available @ http://www.celeso.com/download

#### **ENVIRONMENTAL**

4.90 [124,5]

Enclosure	NEMA 4/4X/6, IP 67
Operating Temperature	40° to 200°F (-40° to 90°C)
Vibration	up to 10 G's to 2000 Hz maximum

### Fig. 1 – Outline Drawing (18 oz. cable tension only)



0.25 [6,4]

DIMENSIONS ARE IN INCHES [MM] tolerances are 0.03 IN. [0.5 MM] unless otherwise noted.

7.87 [199,9] max

→ .105 [4,	$ \underbrace{\frac{0.27}{0.27}}_{\dagger} [6,9] $
5.16 [131,1] max. 4.75 ±0.06 [120,7 ±2,0]	5.30 [134,6]
	* tolerance = +.005001 [+.1303] ** tolerance = +.005005 [+.1313]

A DIMENSION (INCHES)

RANGE

200

300

350

450

eyelet detail

Ø.191 [4,19]\* ∕−Ø.375 [9,52]\*\* 0.58

0.88

1.02

1.17

1.31

MEASURING CABLE in. ∅.047 in. ∅.

0.59

0.79

1.18

1.38

1.77

0.64 [16,3]

mounting hole detail

0.49

0.98

1.47

1.71

n/a


# PT9DN




The PT9DN communicates via DeviceNET protocol with programmable controllers in factories and harsh environments requiring linear position measurements in ranges up to 550".


As a member of Celesco's innovative family of NEMA 4 rated cable-extension transducers, the PT9DN installs in minutes by simply mounting it's body to a fixed surface and attaching it's cable to the movable object. Perfect parallel alignment not required.

## Output Signal



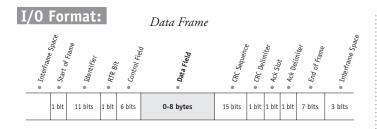

## Data Field



B<sub>0</sub> = LSB current measurement byteB<sub>1</sub> = MSB current measurement byte

B<sub>2</sub> = LSB full stroke range byteB<sub>3</sub> = MSB full stroke range byte

**B**<sub>4</sub> - **B**<sub>7</sub> = not use

#### \*Current Measurement Count

The Current Measurement Count (CMC) is the output data that indicates the present position of the measuring cable.

The CMC is a 16-bit value that occupies the first two bytes ( $B_0$  and  $B_1$ ) of the data field.  $B_0$  is the LSB (least significant byte) and  $B_1$  is the MSB (most significant byte).

The CMC starts at 0000H with the measuring cable fully retracted and continues upward to the end of the stroke range stopping at FFFFH. This holds true for all ranges.

#### \*\*Full Stroke Range

The Full Stroke Range (FSR) is a 16-bit value in the data field that expresses the full range of the sensor in inches. This value can be used to convert the actual count to units of measurement should the application require it.

The full stroke measurement range occupies the second two bytes ( $B_2$  and  $B_3$ ) of the data field.

 $\mbox{\sc B}_2$  is the LSB (least significant byte) and  $\mbox{\sc B}_3$  is the MSB (most significant byte).

This value is expressed in inches.

#### Example:

Hex Value	Decimal Equivalent	Full Stroke Range
001E	30	30 inches

#### Converting CMC to Inches

If required, the CMC can easily be converted to a linear measurement expressed in inches instead of just counts.

This is accomplished by first dividing the CMC by 65,535 (total counts over the range) and then multiplying that value by the FSR:

$$\left(\begin{array}{c} \text{CMC} \\ \hline 65,535 \end{array}\right)$$
 X FSR

#### Example:

If the full stroke range is **30 inches** and the current position is **OFF2 Hex** (4082 Decimal) then,

$$\left(\frac{4082}{65,535}\right)$$
 X 30.00 inches = 1.87 inches

#### Address Setting (Node ID), Baud Rate and Bus Termination Settings

#### Address Setting (Node ID)

The Address Setting (Node ID) is set via 6 switches located on the 8-pole DIP switch found on the DeviceNET controller board located inside the transducer.

The DIP switch settings are binary starting with switch number  ${\bf 1}$  (=  $2^0$ ) and ending with switch number  ${\bf 6}$  (=  $2^5$ ).

<b>DIP-1</b> (20)	<b>DIP-2</b> (2 <sup>1</sup> )	<b>DIP-3</b> (2 <sup>2</sup> )	<b>DIP-4</b> (2 <sup>3</sup> )	<b>DIP-5</b> (2 <sup>4</sup> )	<b>DIP-6</b> (2 <sup>5</sup> )	address (decimal)	
0	0	0	0	0	0	0	
1	0	0	0	0	0	1	
0	1	0	0	0	0	2	
•••		•••	•••	•••		•••	
1	1	1	1	1	1	63	
↑ = "0" 12345678							

#### **Baud Rate**

The transmission baud rate may be either factory preset at the time of order or set manually at the time of installation.


The baud rate can be set using switches **7** & **8** on the 8-pole DIP switch found on the DeviceNET controller board located inside the transducer.

DIP-7	DIP-8	baud rate		
0	0	125k		
1	0	250k		
0	1	500k		
1	1	125k		
0 1 500k				


#### **Bus Termination**

The setting of the internal bus termination resistor may be specified upon order or manually changed by the end user at the time of installation.


The bus termination resistor is activated setting switches 1 & 2 on the 2-pole DIP switch (located on the internal DeviceNET controller board) to the "ON" position.




#### **DeviceNET Controller Board and DIP Switch Location**









internal dip switches & controller board

to gain access to the controller board, remove four Allen-Head Screws and remove end cover

# PT9DN • Cable-Extension Transducer: DeviceNET®

# Ordering Information:

# **Model Number:**

Sample Model Number:

PT9DN - 200 - AL - N34 - 26 - FR - 500 - TR - SC5

→ range: 200 inches

R range:
A enclosure
B measuring cable:

aluminum .034 nylon-coated stainless 18 oz.

measuring cable tension:

action cable exit:
baud rate:
terminating resistor:
electrical connection:

18 oz.
front (horize
front

18 oz. front (horizontal) 500 k bits/sec. yes 5-meter cordset with straight plug

Full Stroke Range:

R order code:	75	100	150	200	250	300	350	400	450*	500*	550*	
full stroke range, min:	75 in.	100 in.	150 in.	200 in.	250 in.	300 in.	350 in.	400 in.	450 in.	500 in.	550 in.	_

\* – 36 oz. cable tension strongly recommended

# **Enclosure Material:**

♠ order code:ALSSpowder-painted aluminum303 stainless

# **Measuring Cable:**

© order code: N34 S47 V62

0.034-inch nylon-coated stainless steel available in all ranges all ranges up to 500 inches


N34 S47 V62

0.062-inch thermoplastic all ranges up to 500 inches all ranges up to 400 inches

# Measuring Cable Tension:

<b>@</b> order code:		26	52	
tension (30%):	1	8 oz.	36 o	Z.
enclosure material:	aluminum	stainless steel	aluminum	stainless steel
max. acceleration:	1 G	.33 G	5 G	2 G
max. velocity:	60 inches/sec	20 inches/sec	200 inches/sec	80 inches/sec
		standard housing see fig 1.		dual-spring housing see fig 2.

# Cable Exit:

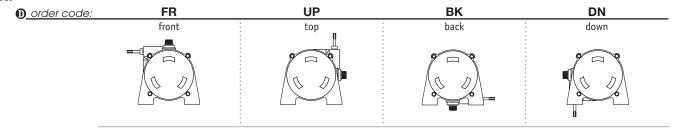

## **Baud Rate:**

<b>B</b> order code:	125	250	500
	125 kbaud	250 kbaud	500 kbaud

## Ordering Information:

# **Terminating Resistor:**


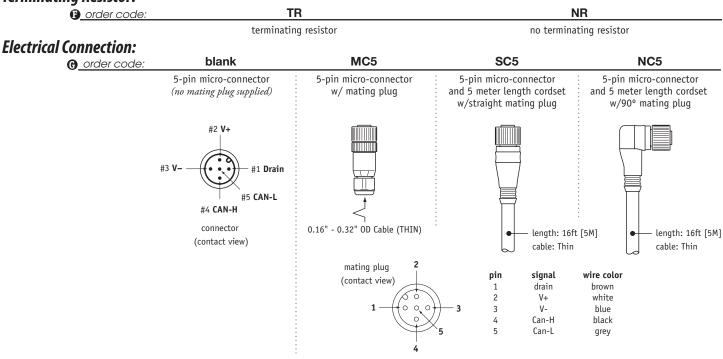


Fig. 2 – Outline Drawing (36 oz. cable tension only)



version: **6.0** last updated: **August 30, 2011**  $PT9DN \mid 142$ 

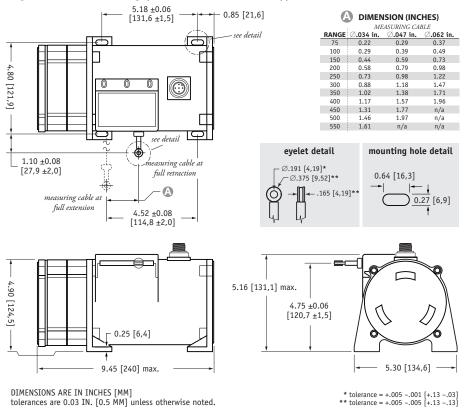